

FIGURE 1

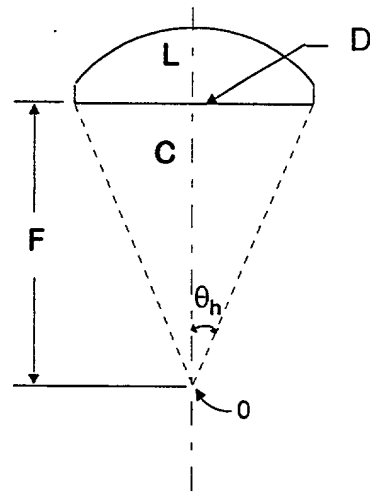


FIGURE 2

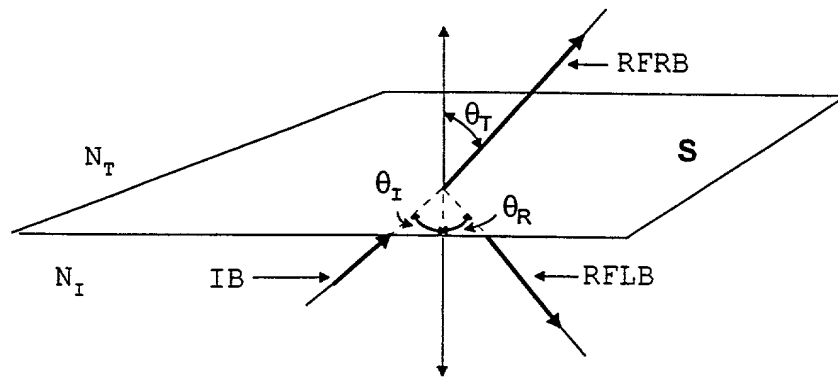


FIGURE 3

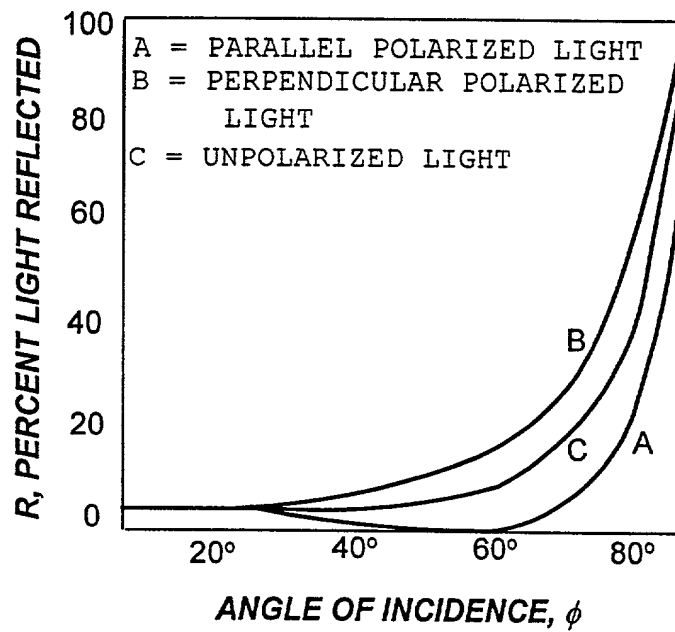


FIGURE 4A

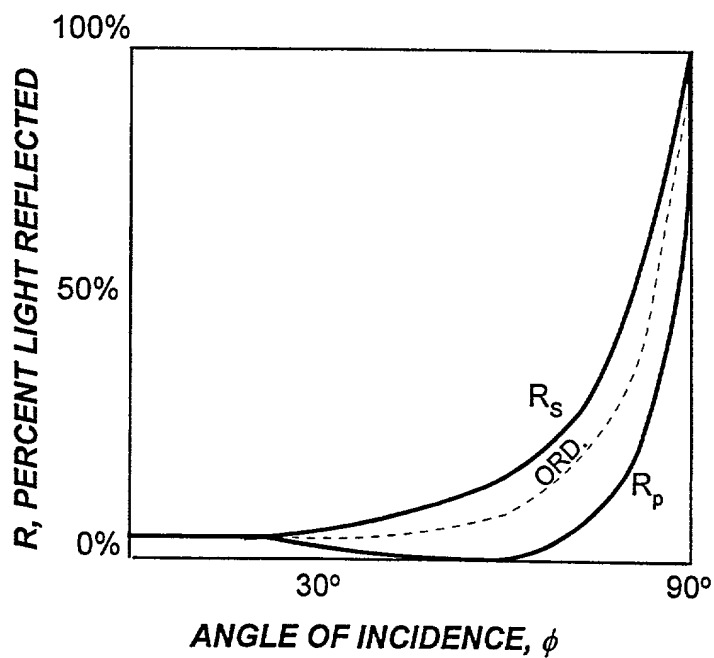


FIGURE 4B

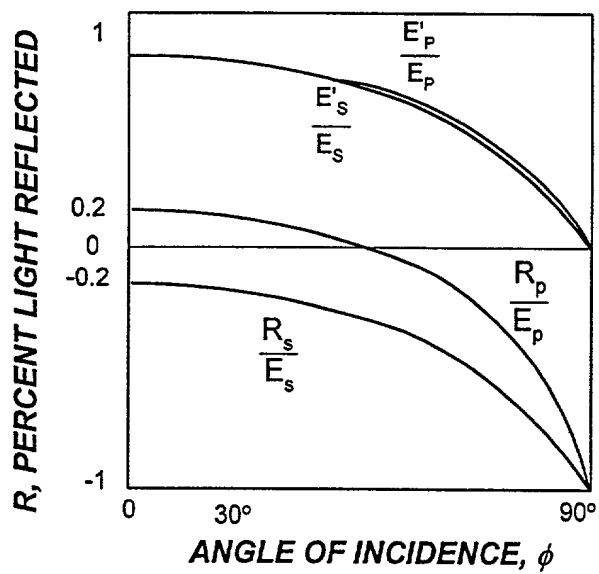


FIGURE 4C

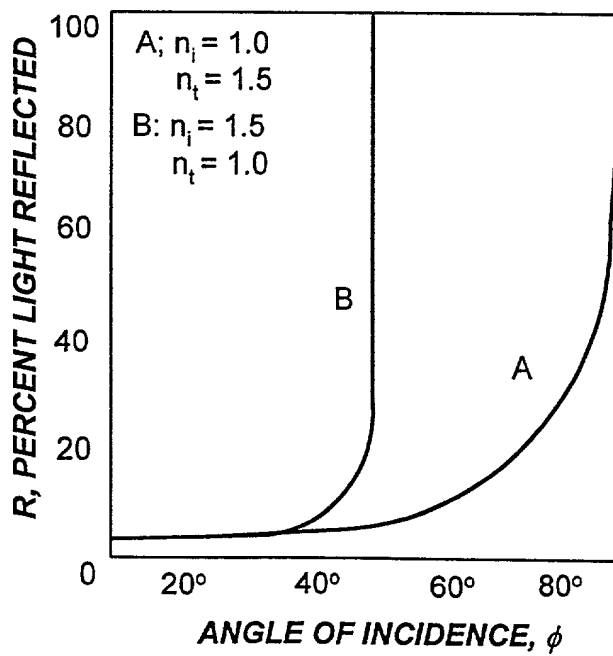


FIGURE 5A

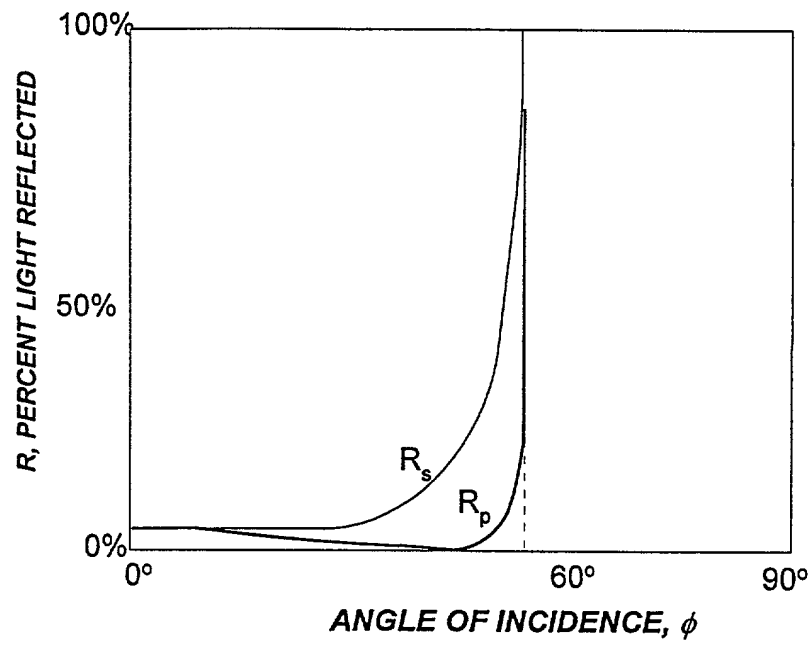


FIGURE 5B

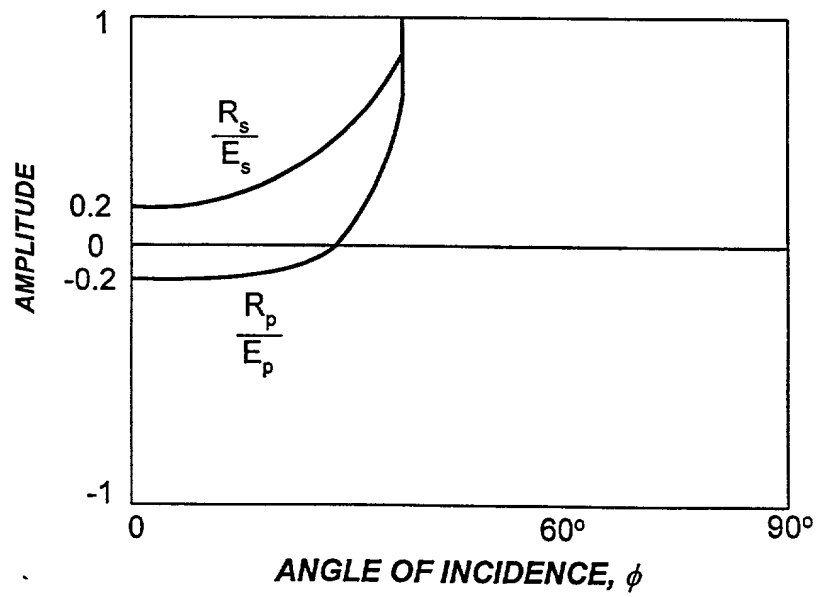


FIGURE 5C

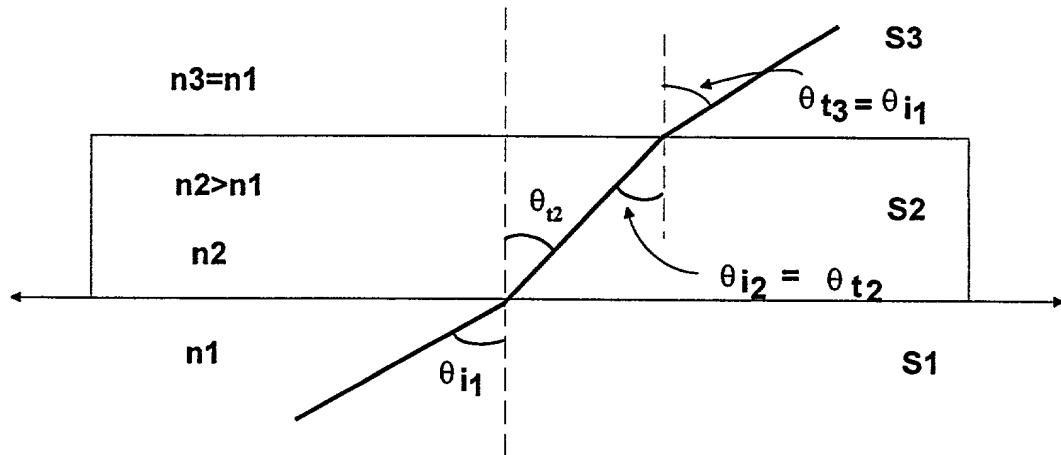


FIGURE 6

$n_i = 1$ $n_t = 1.5$

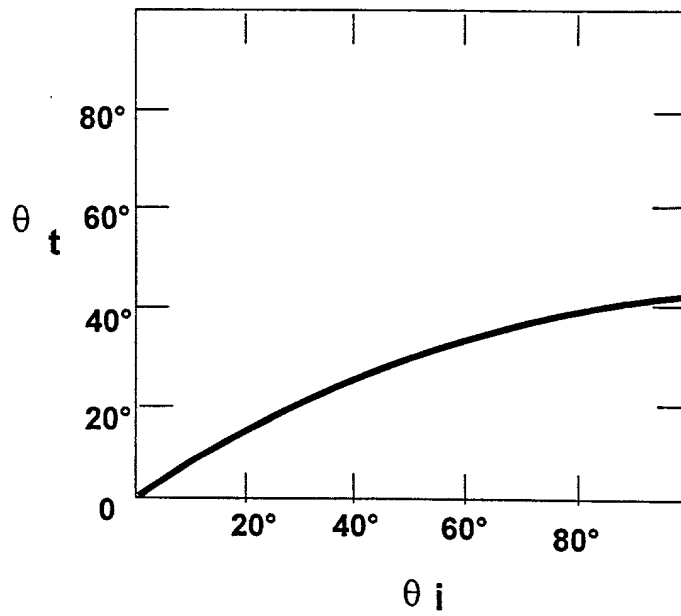


FIGURE 7

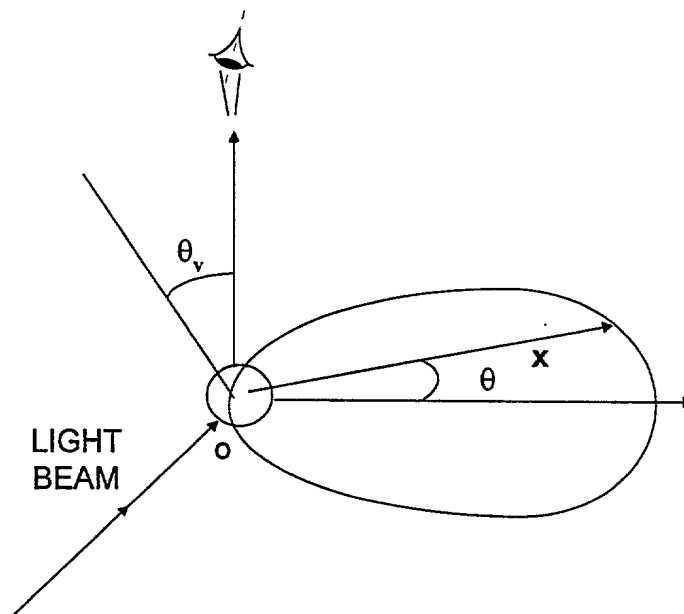


FIGURE 8

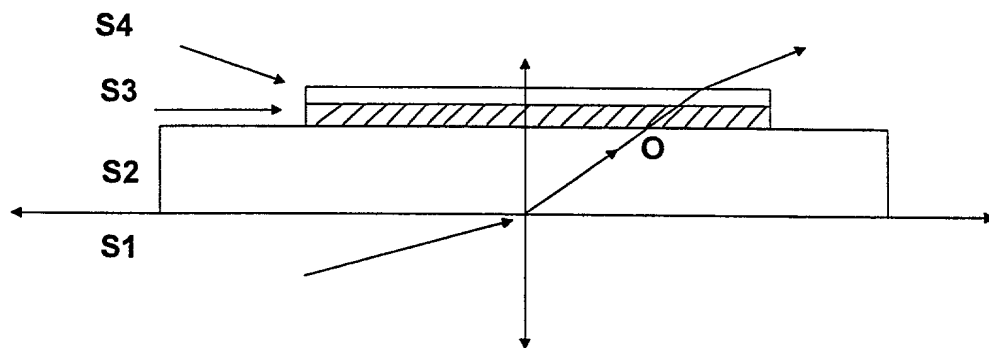


FIGURE 9

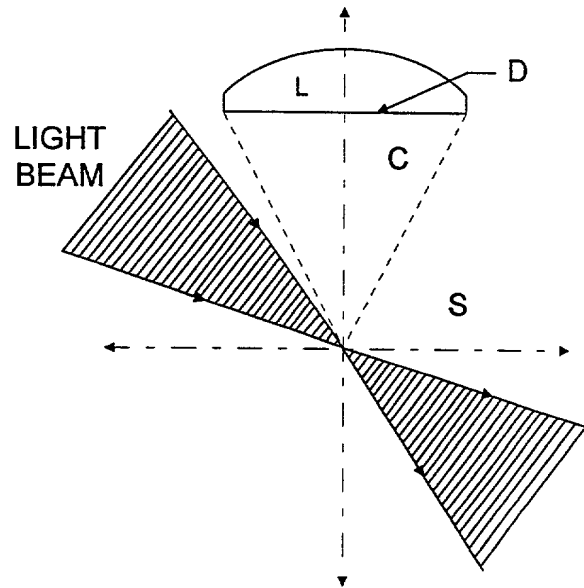


FIGURE 10

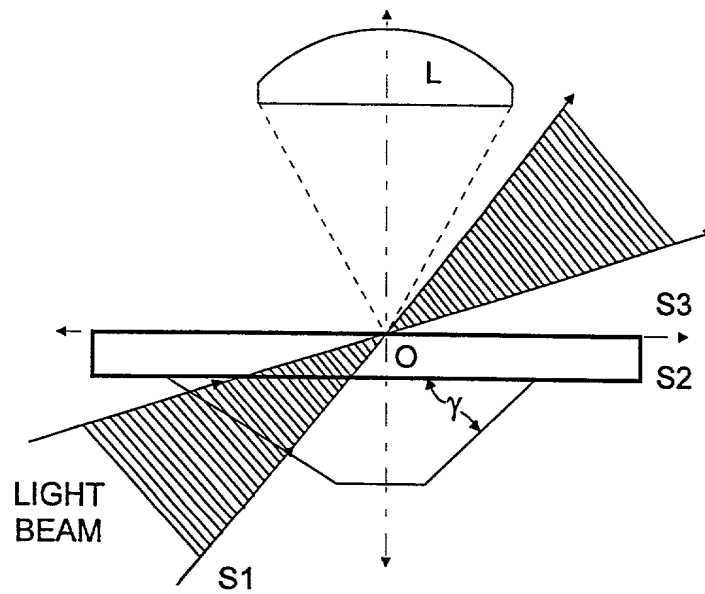


FIGURE 11

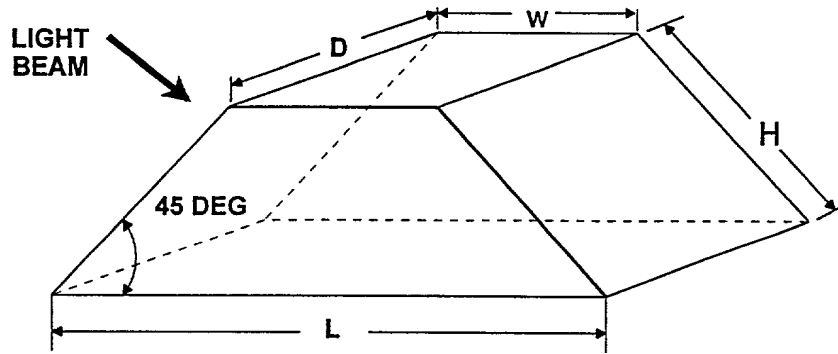


FIGURE 12A

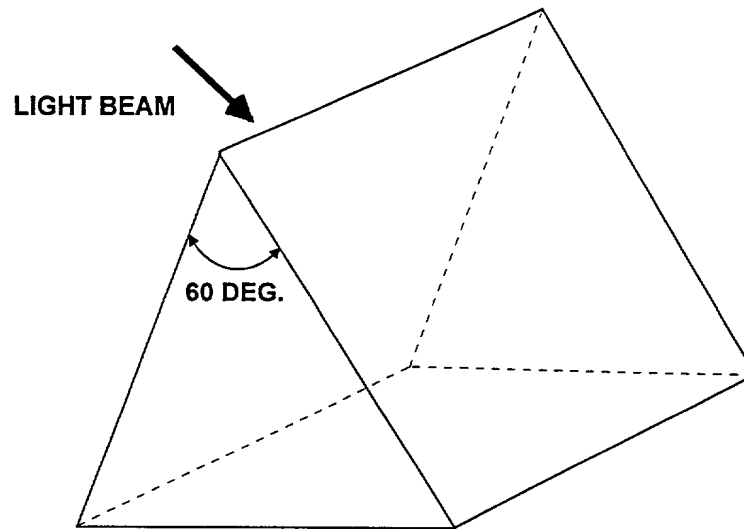


FIGURE 12B

9/30

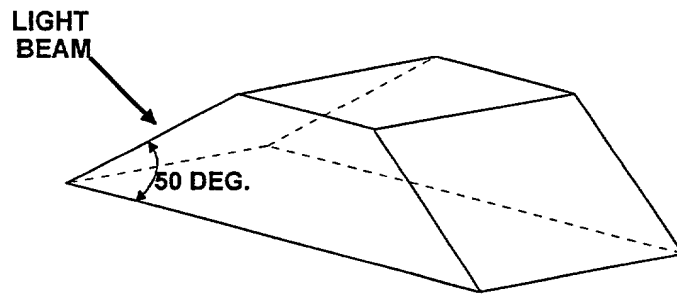


FIGURE 12C


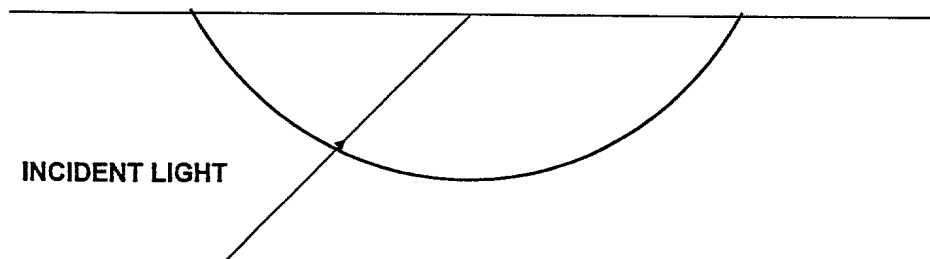


FIGURE 12D

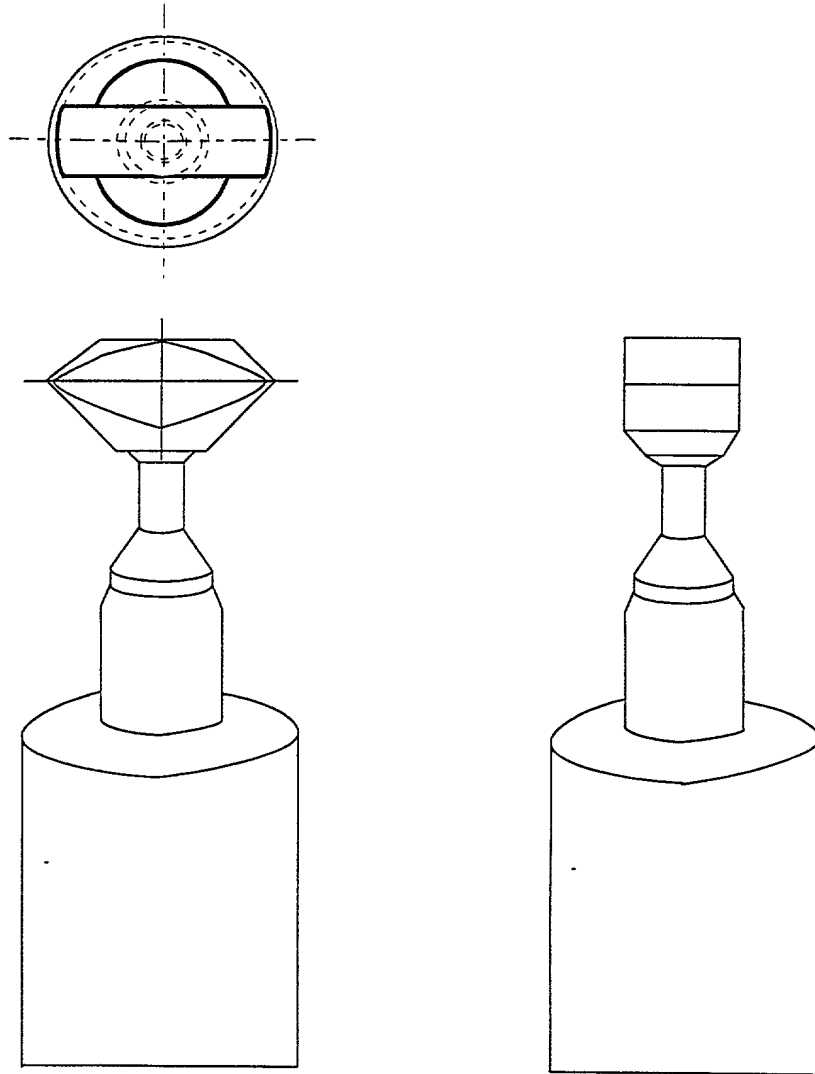

NOT TO SCALE

FIGURE 12E

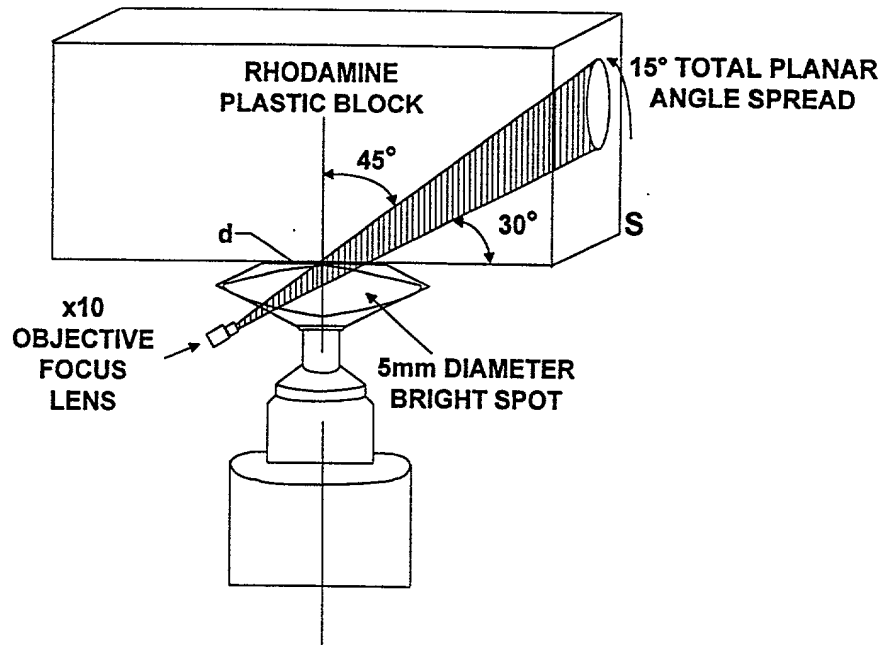


FIGURE 13

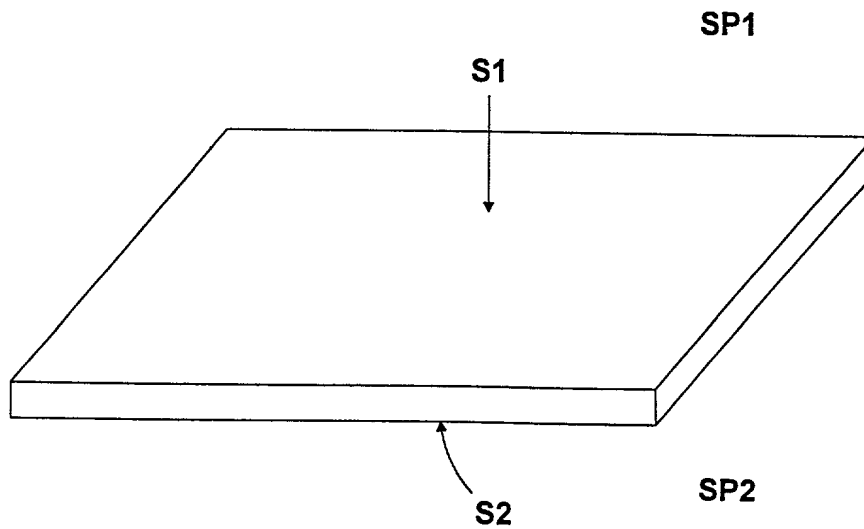


FIGURE 14

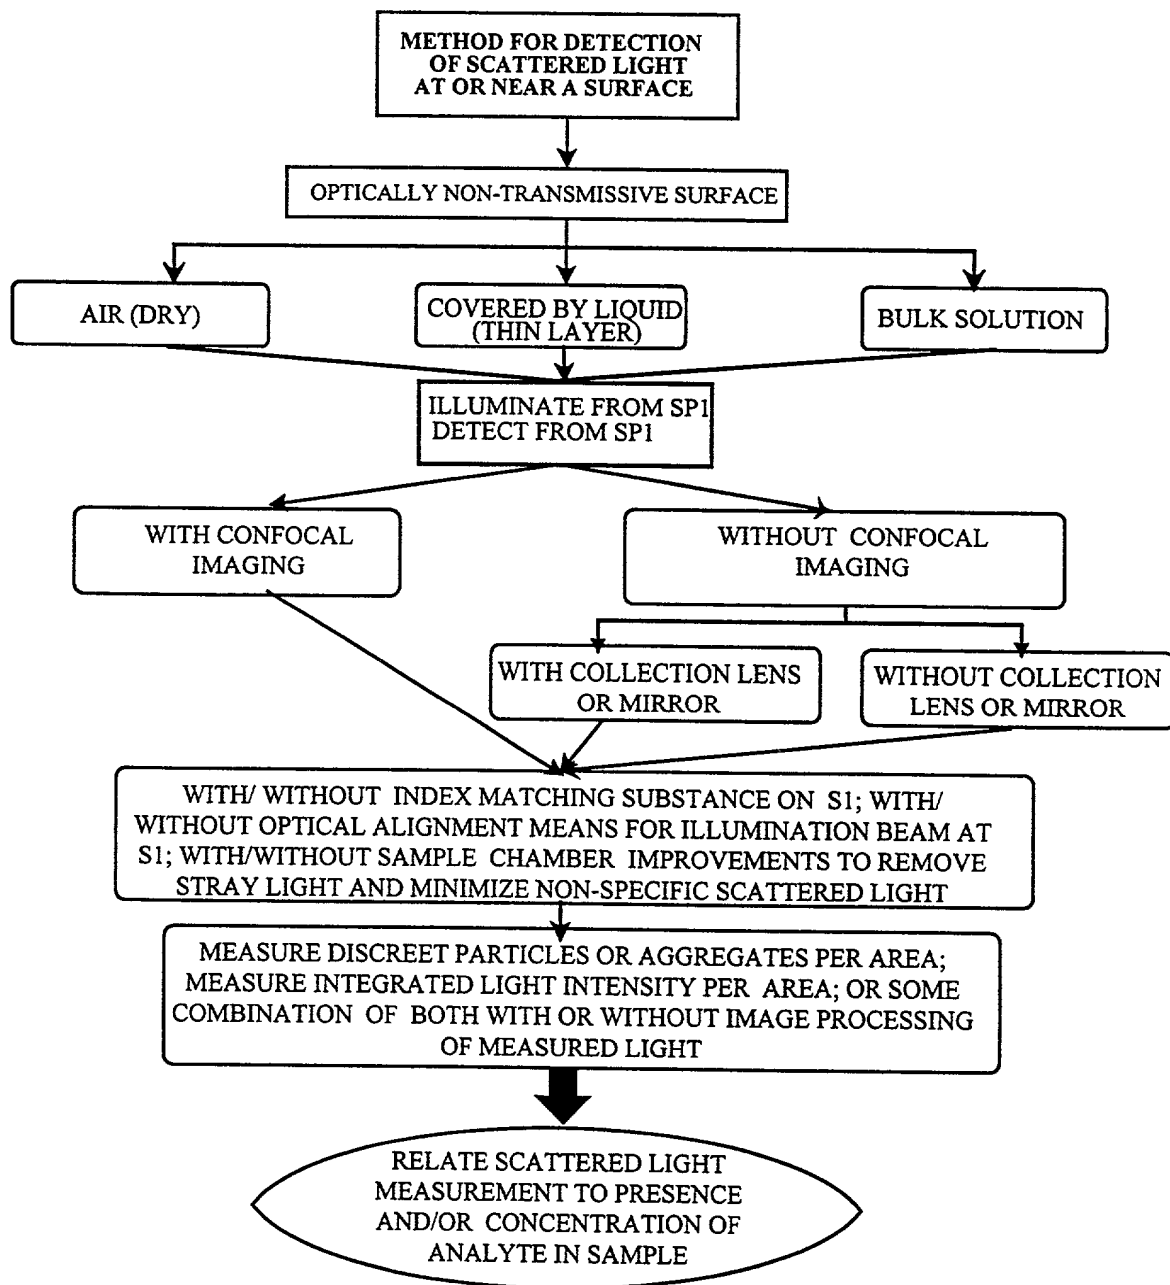


FIGURE 15A

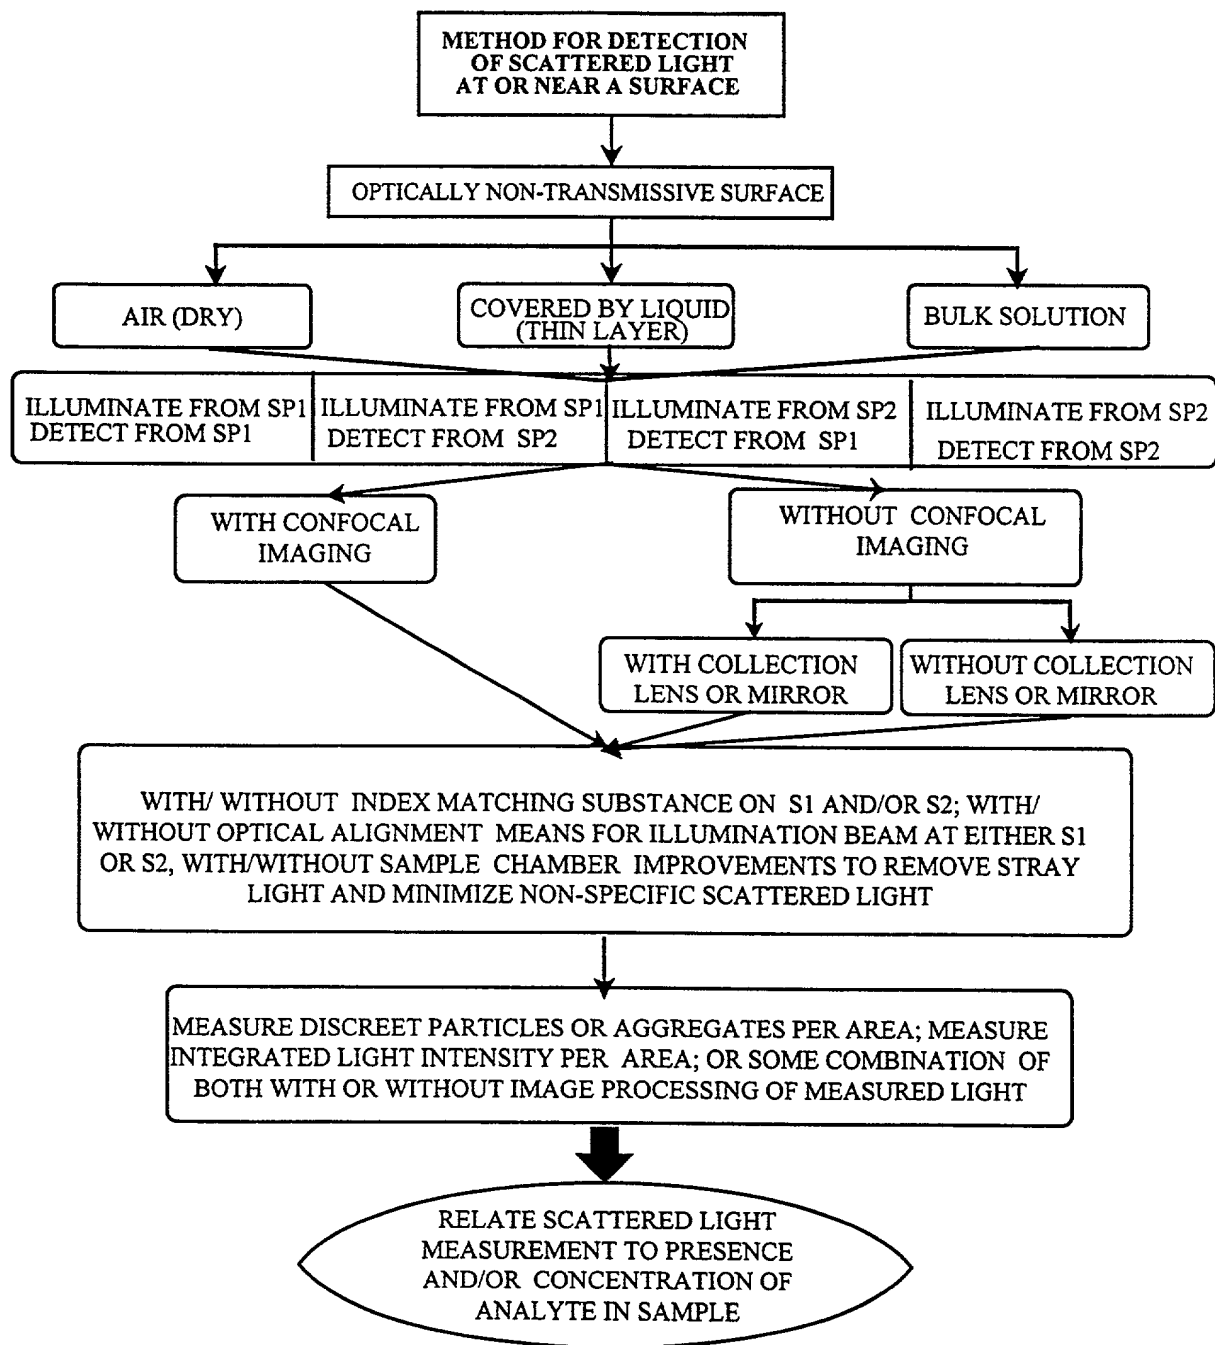


FIGURE 15B

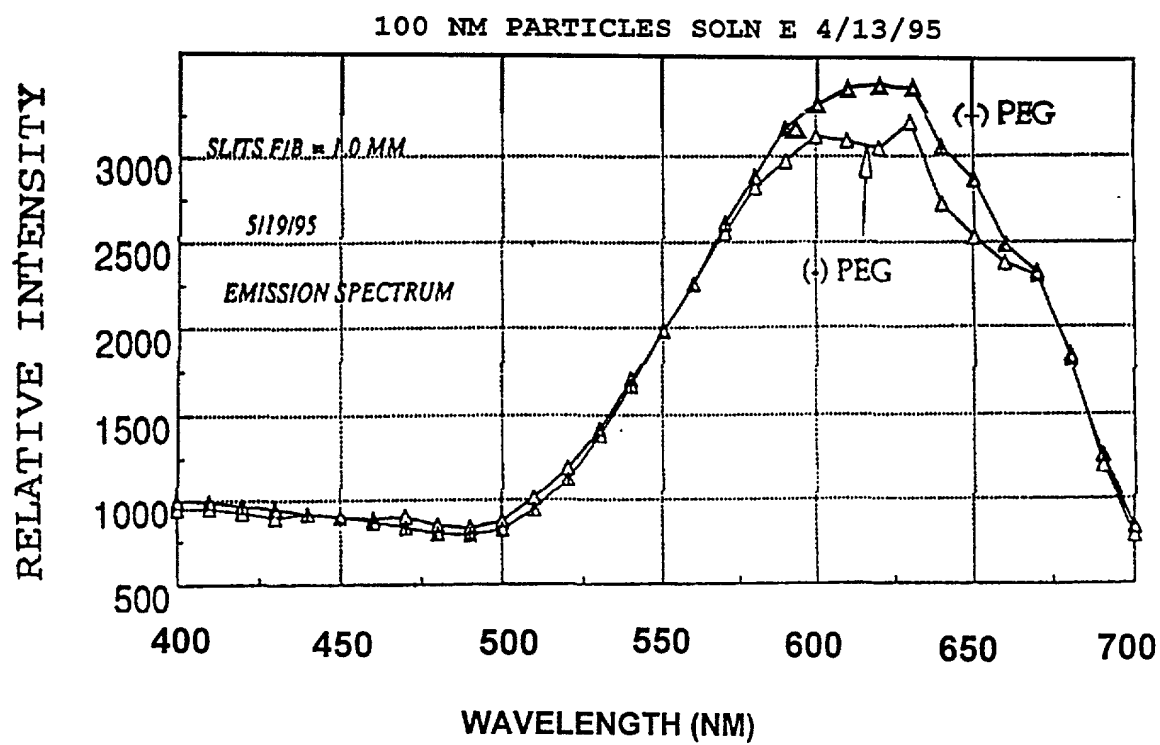


FIGURE 16

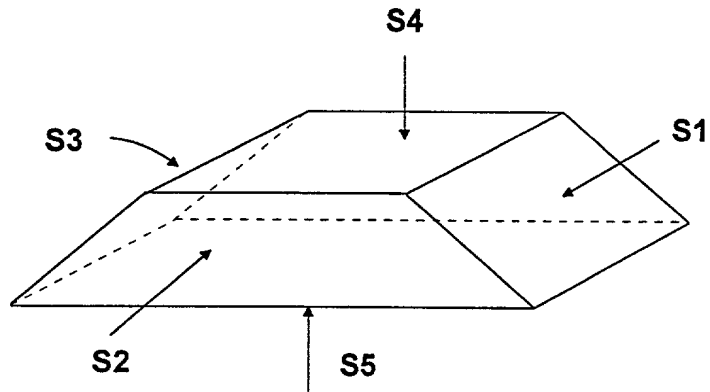


FIGURE 17

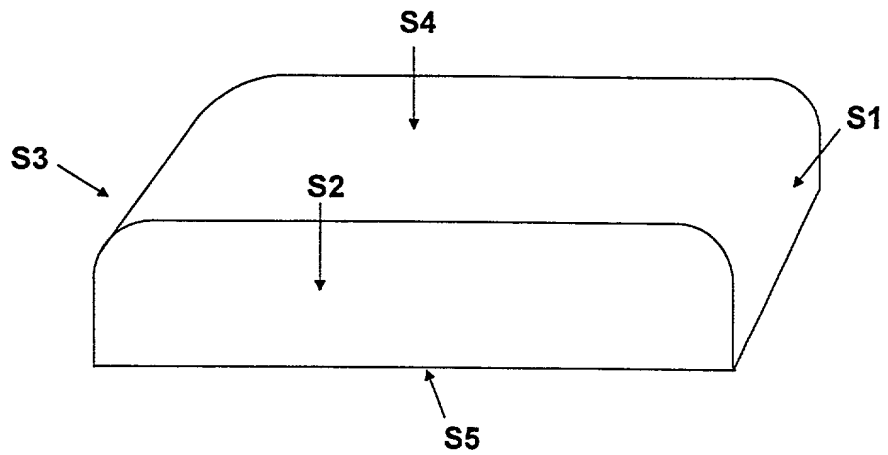


FIGURE 18

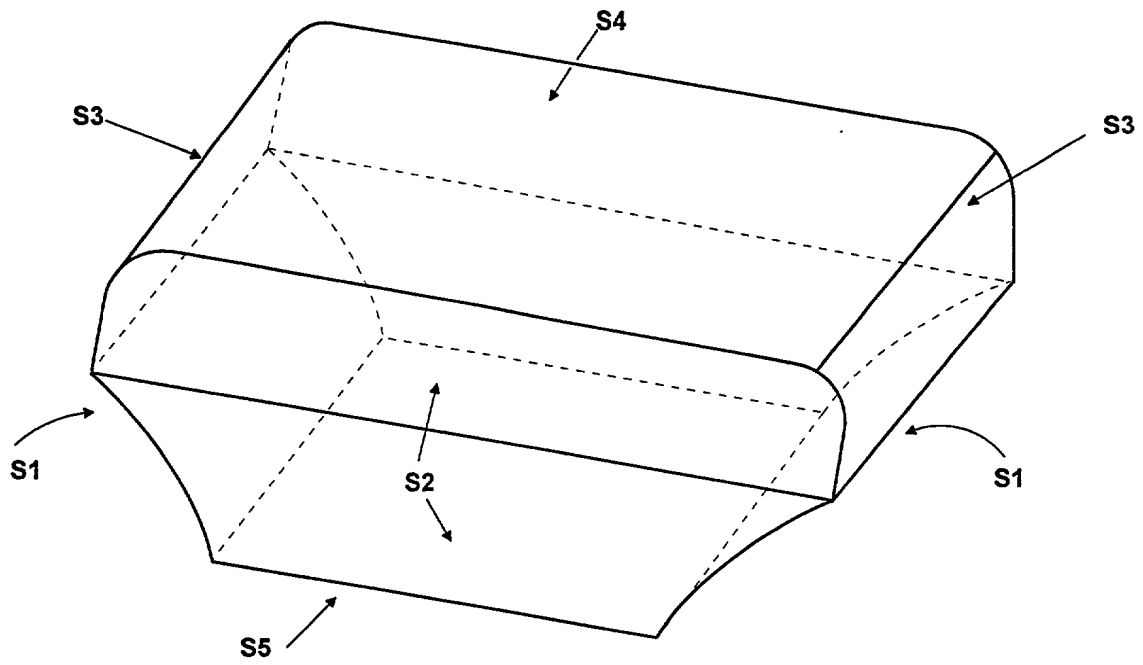


FIGURE 19

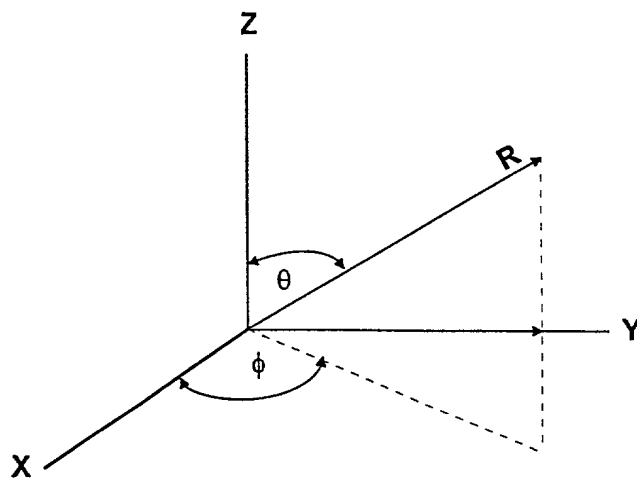


FIGURE 20

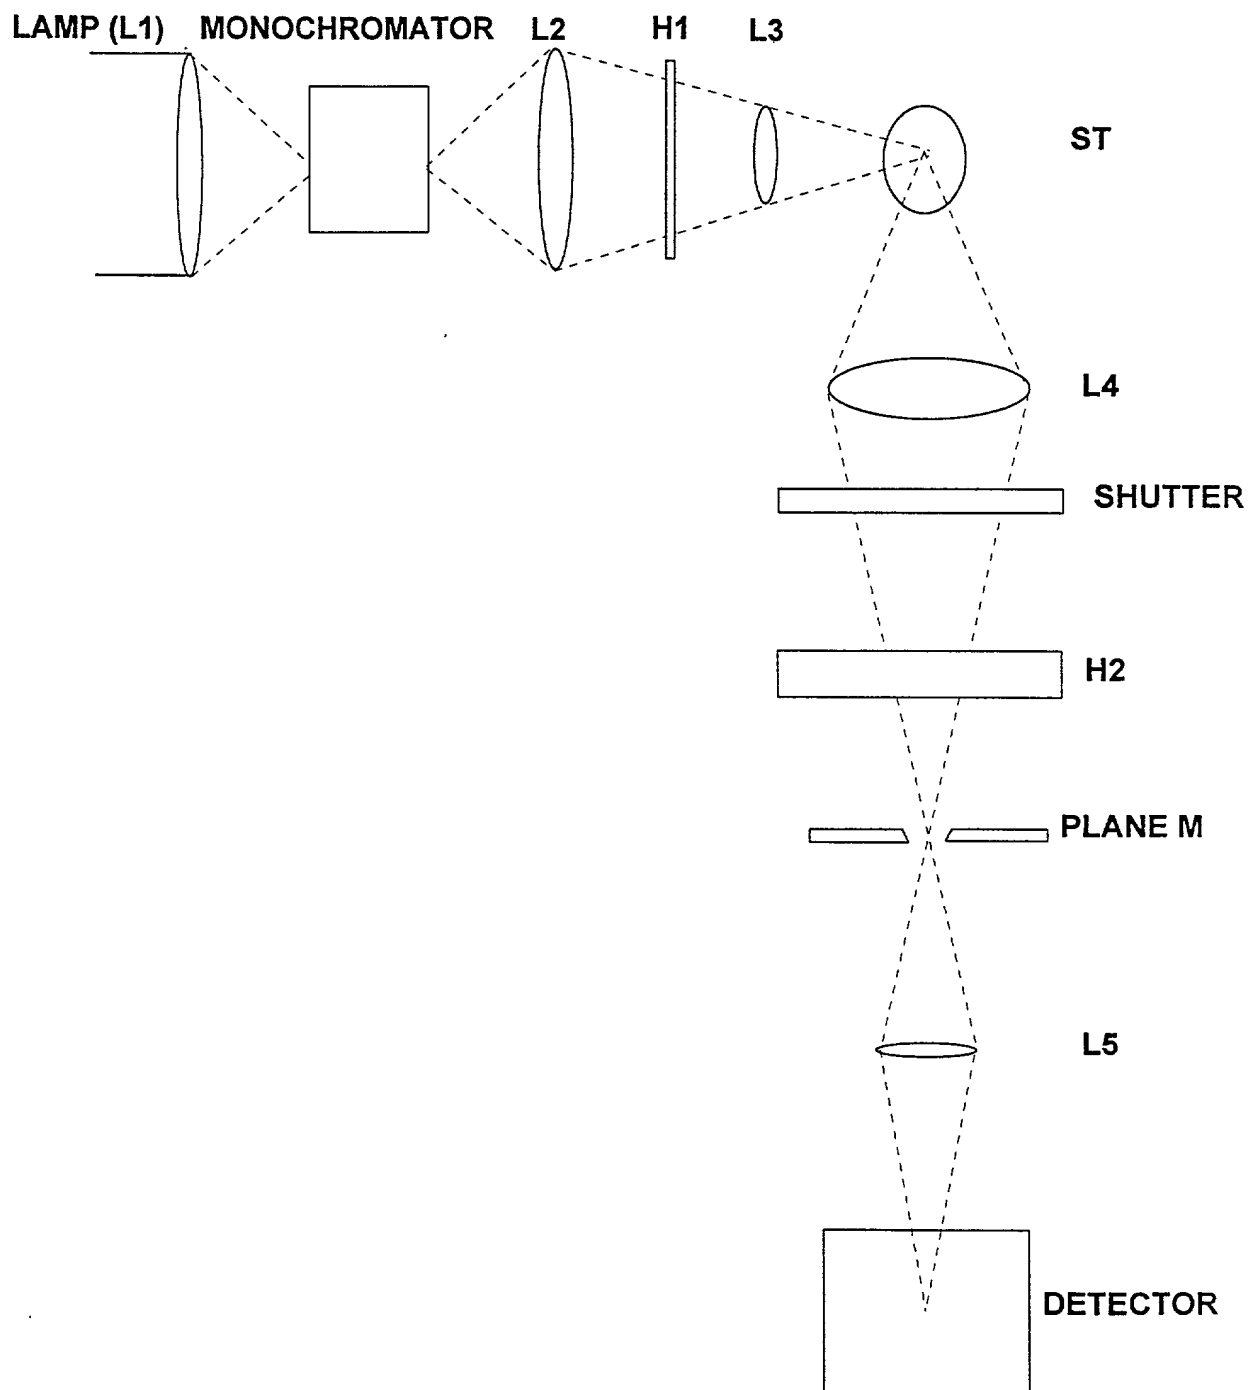


FIGURE 21

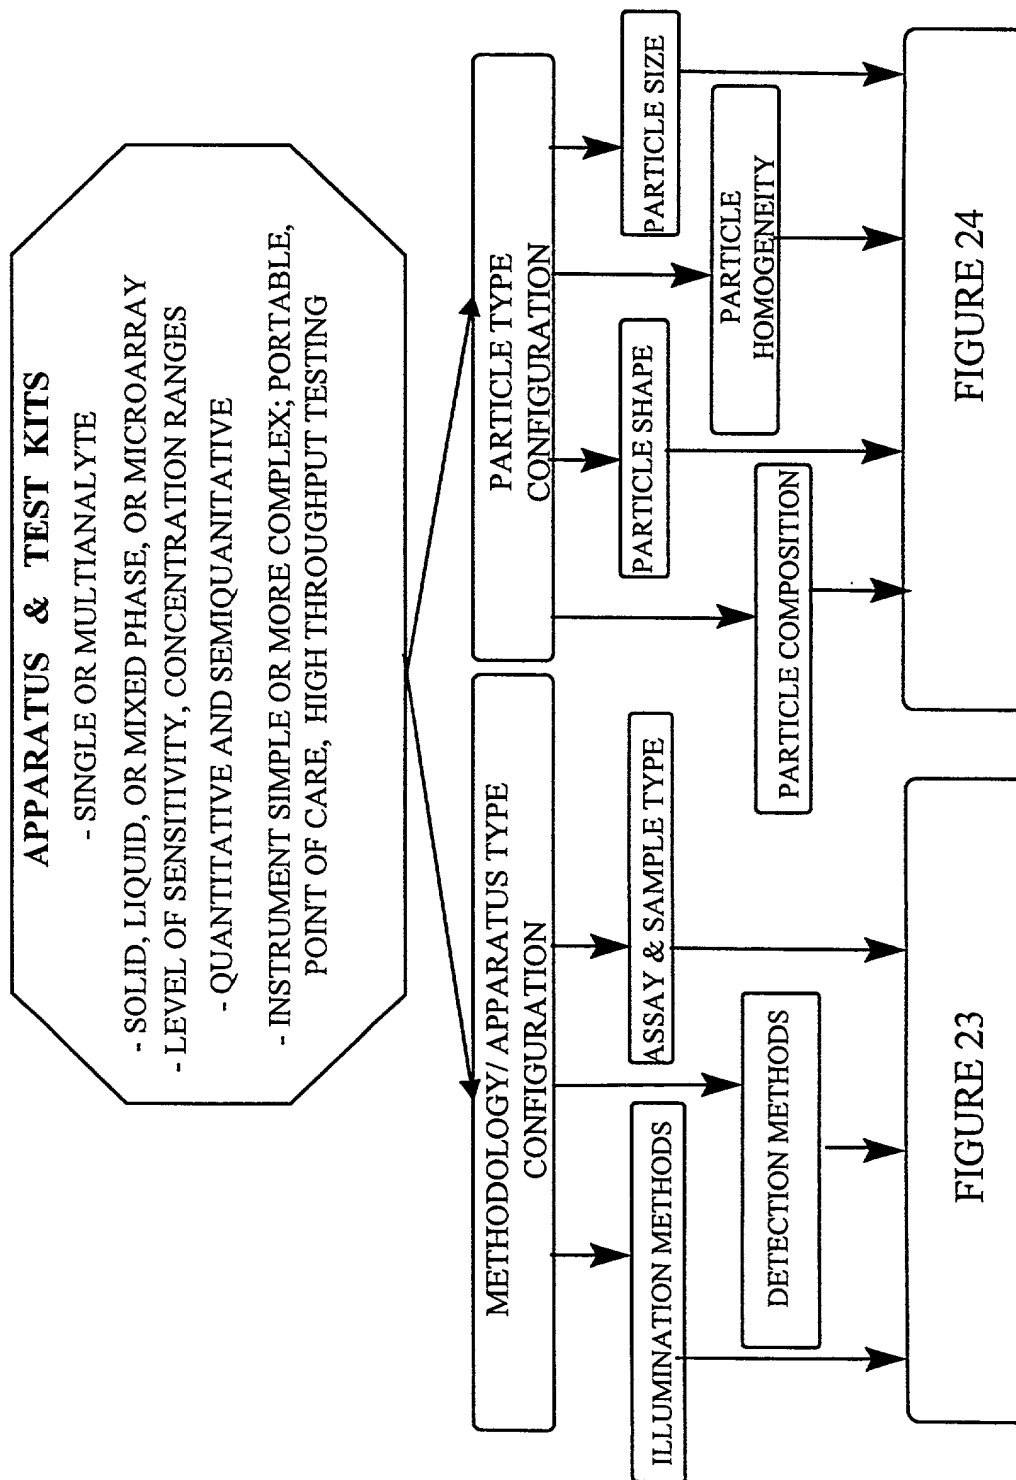


FIGURE 22

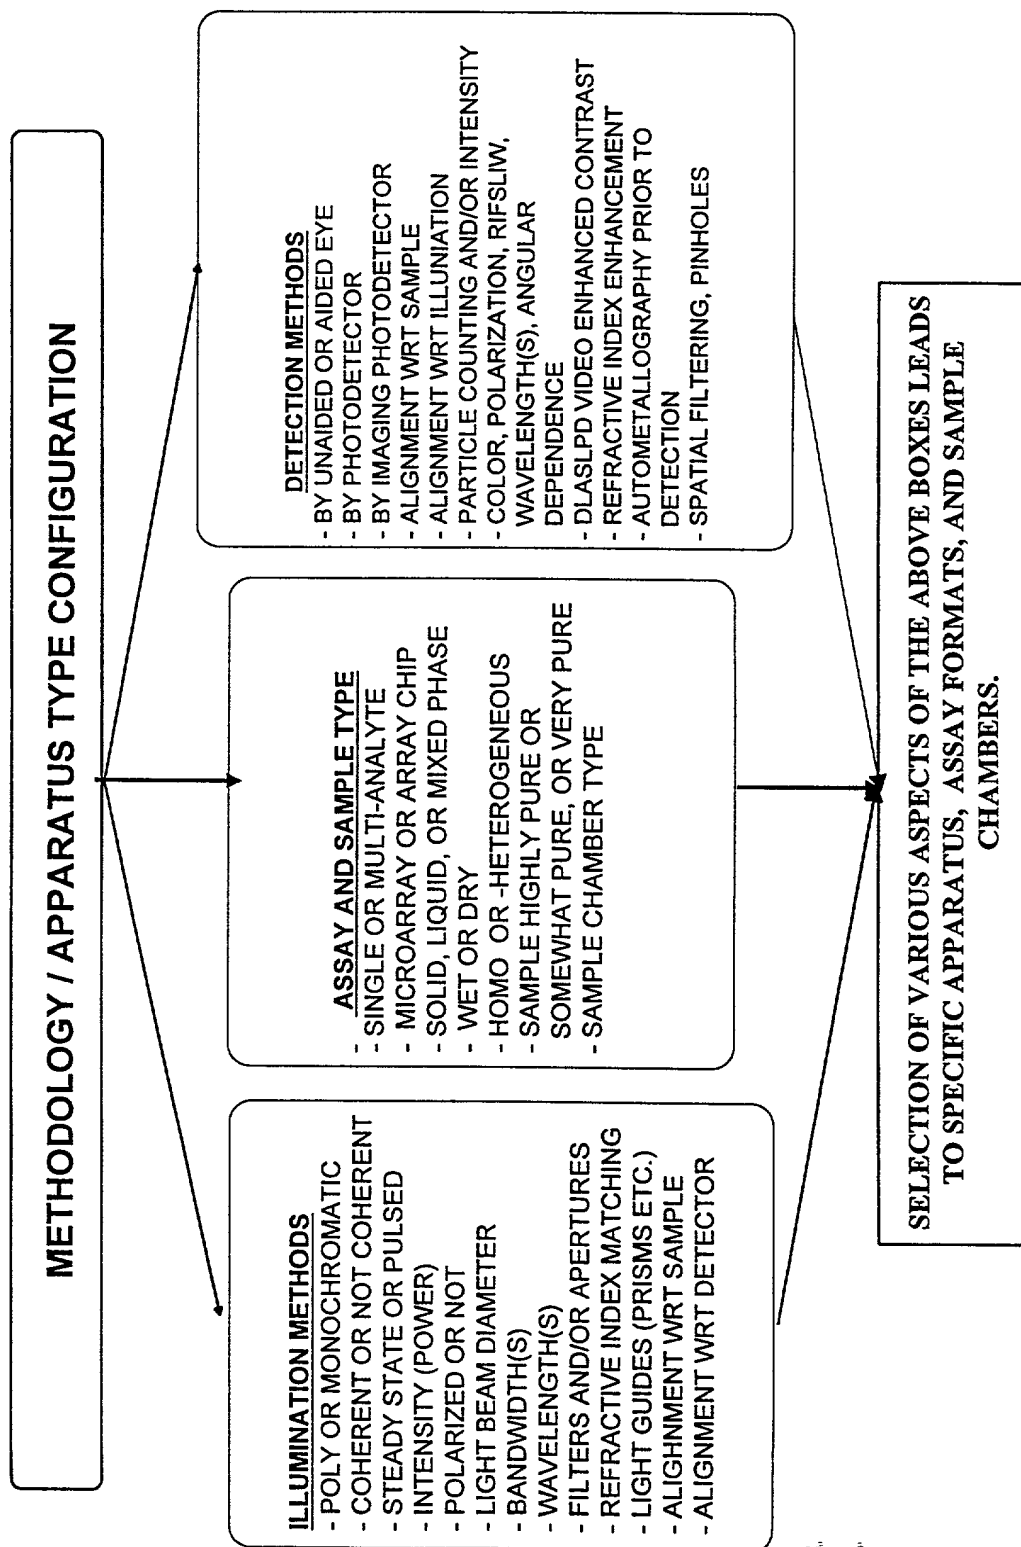


FIGURE 23

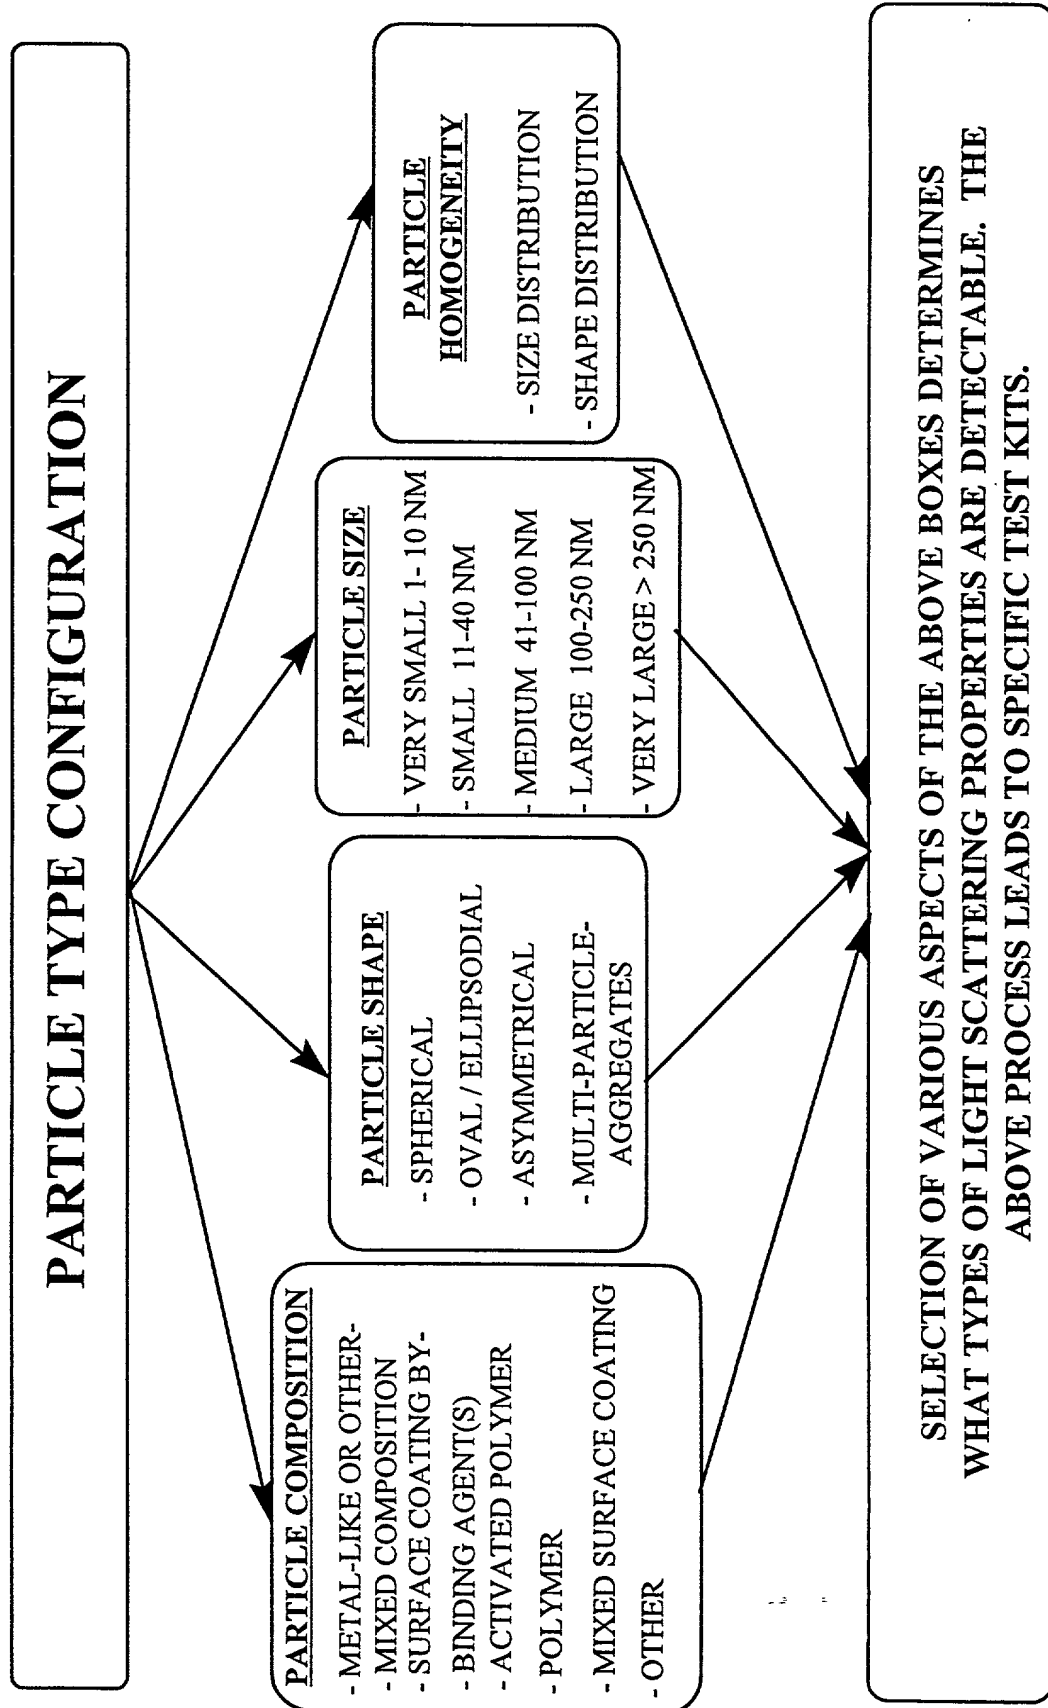


FIGURE 24

**PRACTICE OF INVENTION
TO A SPECIFIC DIAGNOSTIC NEED
LEADING TO SPECIFIC APPARATUS AND
TEST KITS**

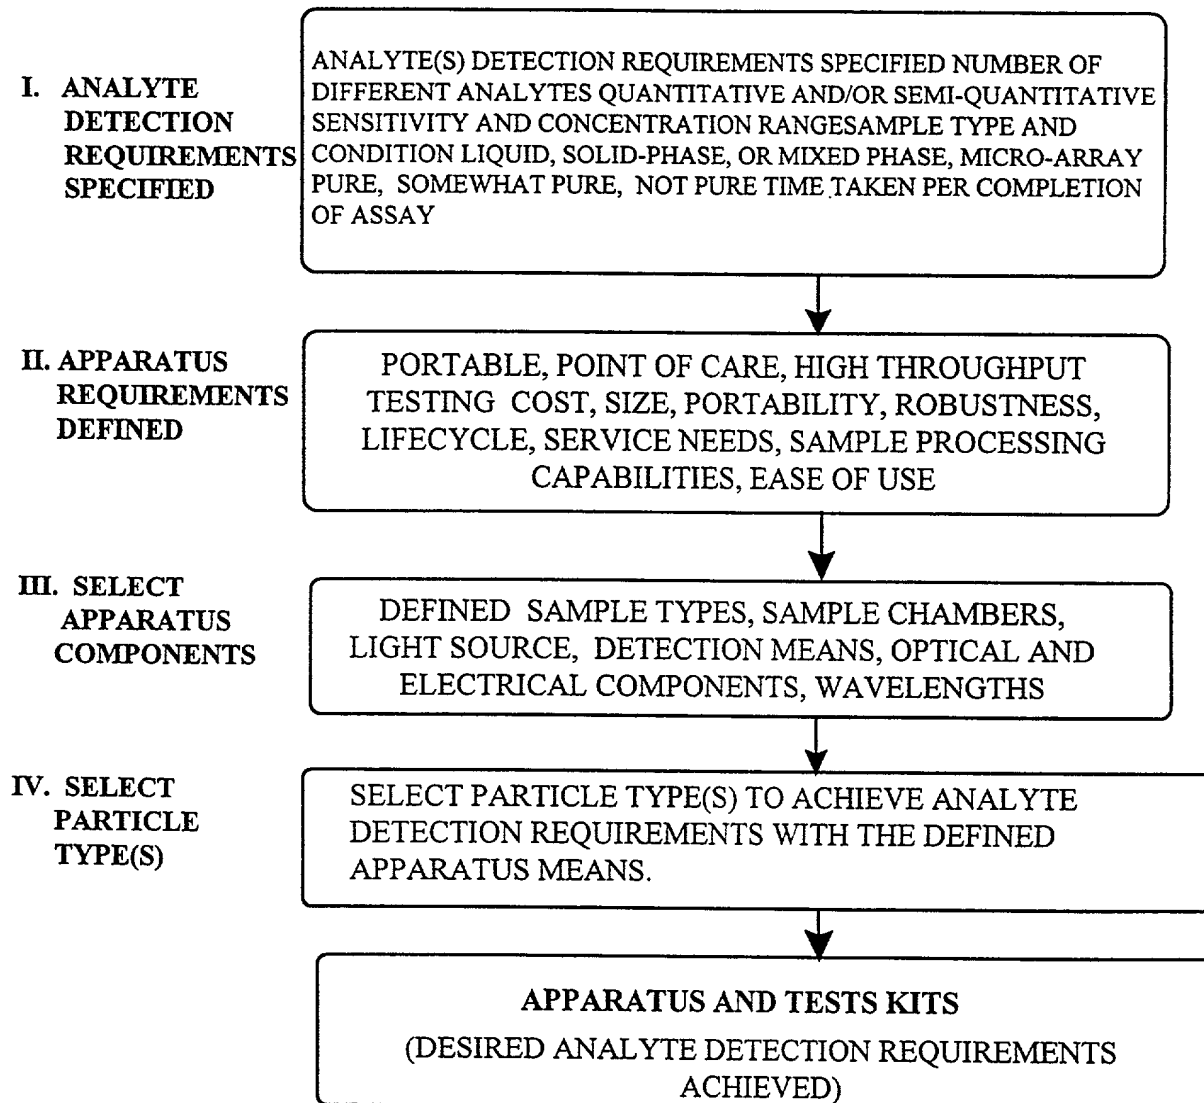
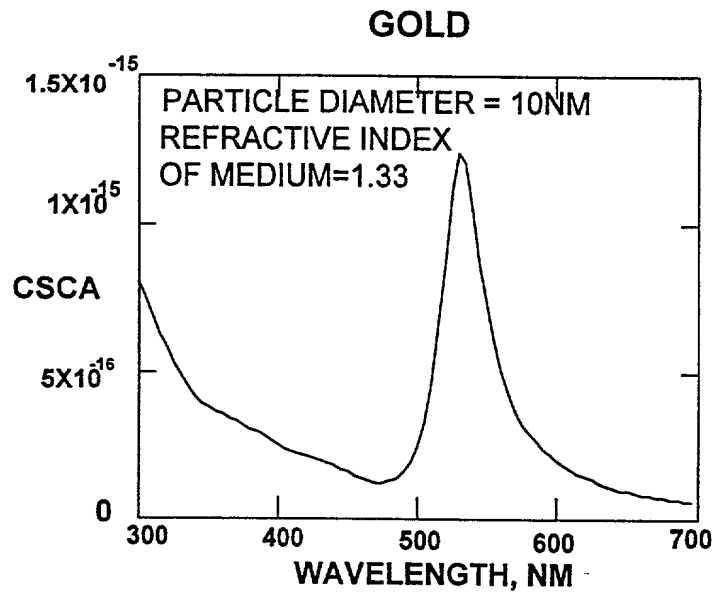
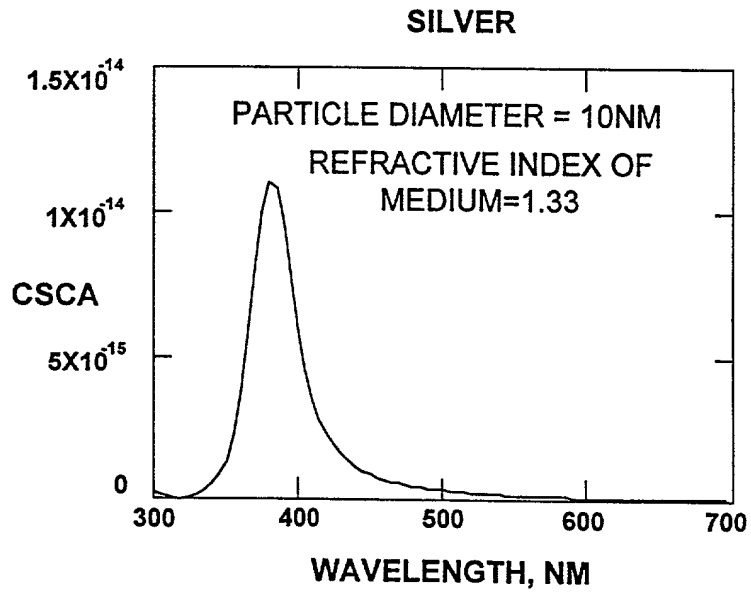
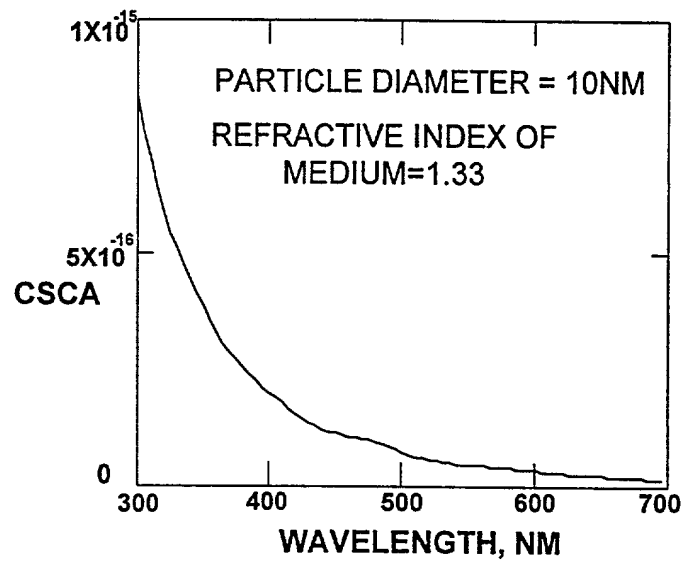
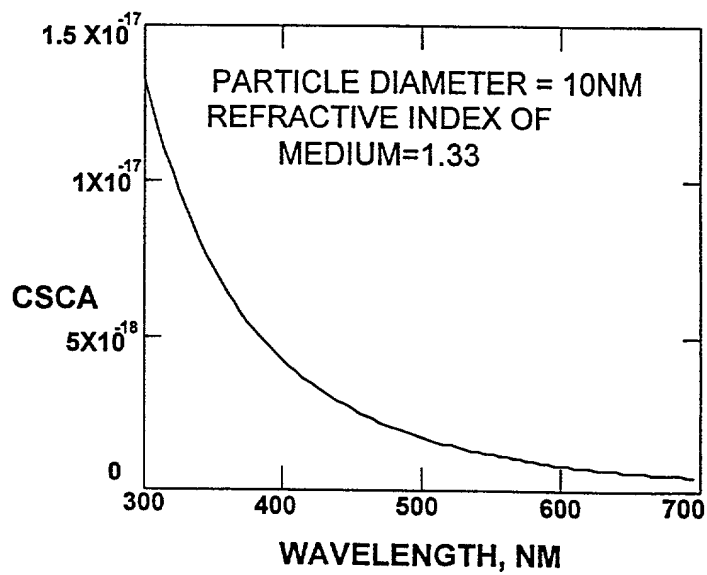
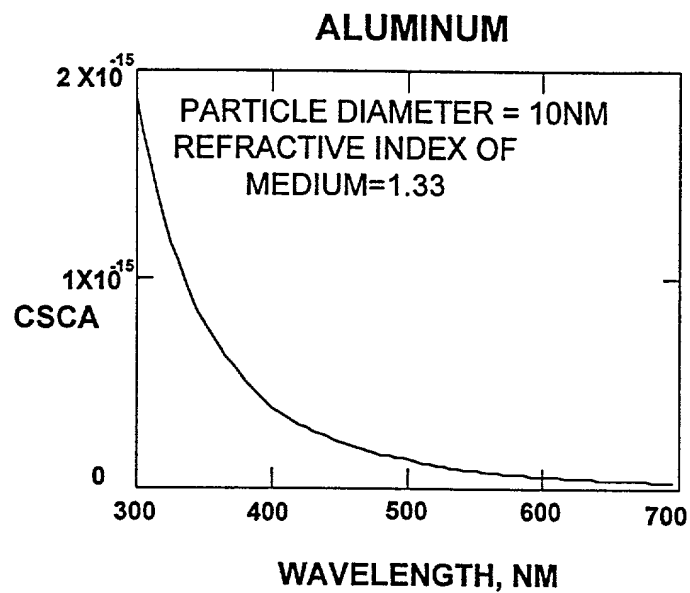
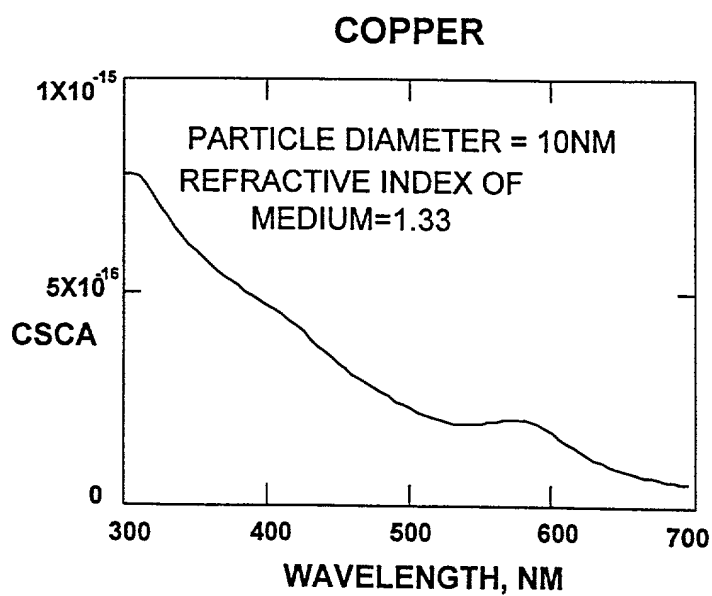


FIGURE 25

**FIGURE 26A****FIGURE 26B**

SELENIUM**FIGURE 26C****POLYSTYRENE****FIGURE 26D**

**FIGURE 26E****FIGURE 26F**

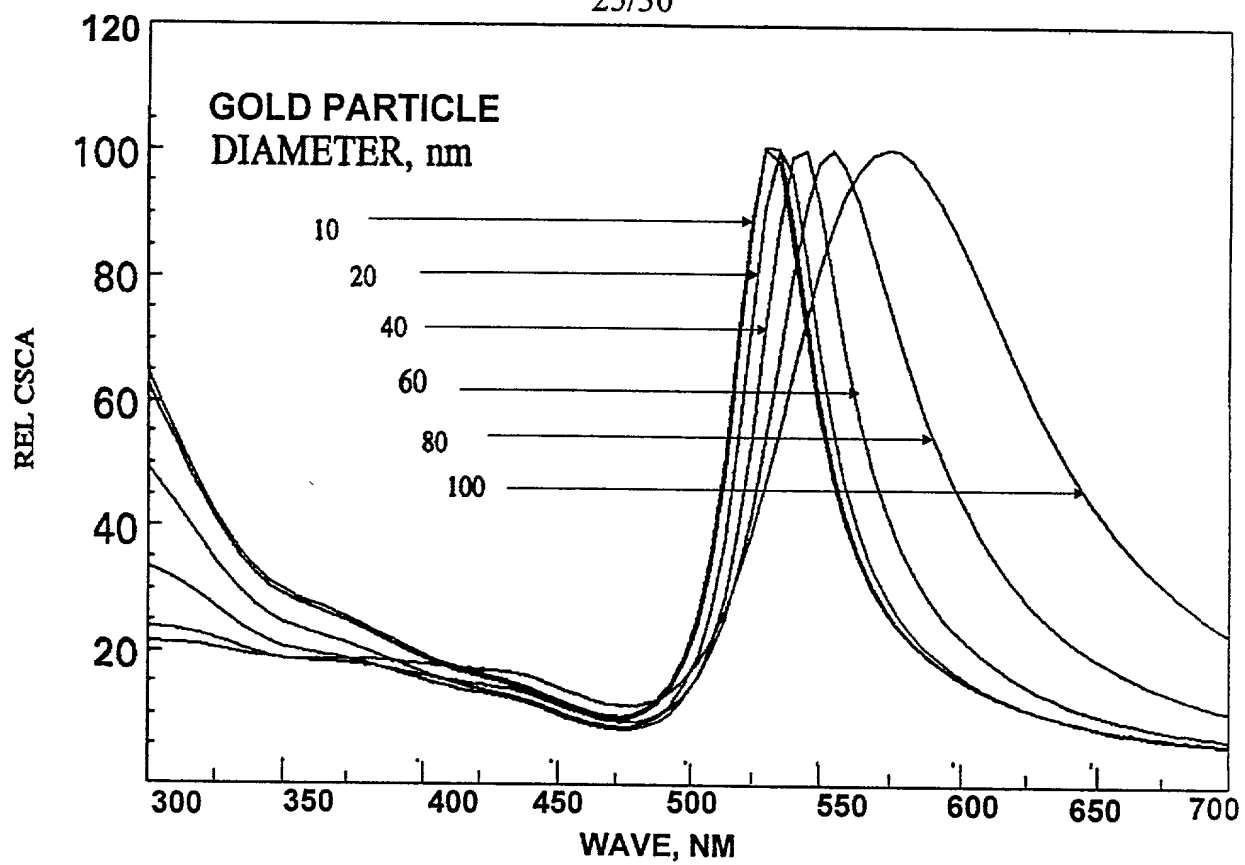


FIGURE 27

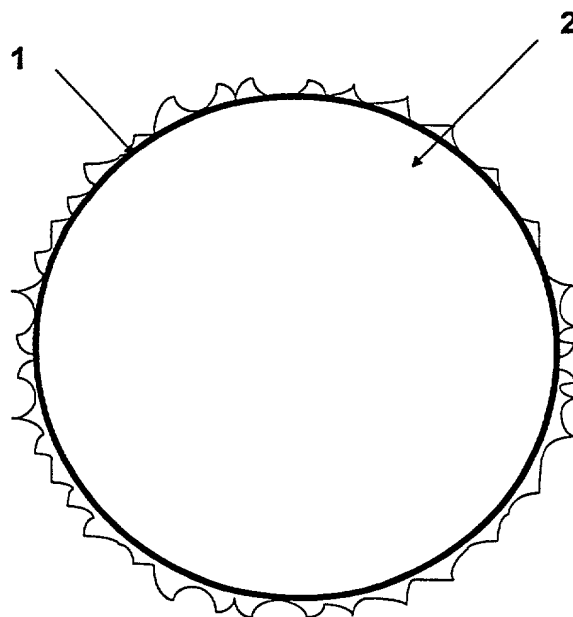


FIGURE 28

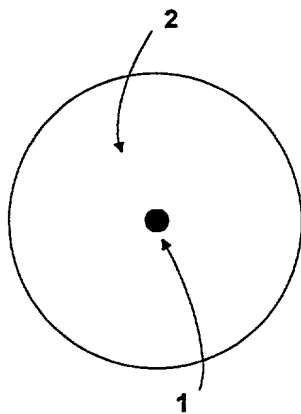


FIGURE 29A

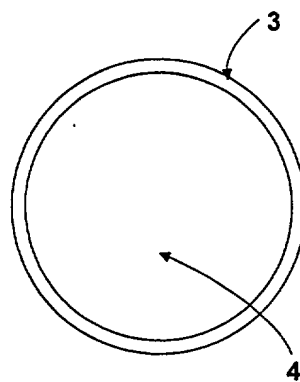


FIGURE 29B

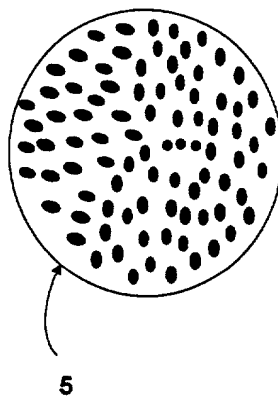


FIGURE 29C

27/30

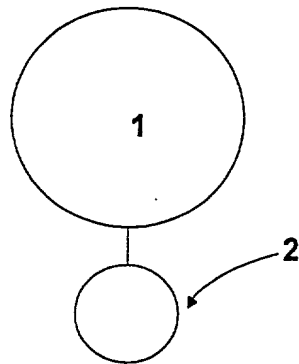


FIGURE 30A

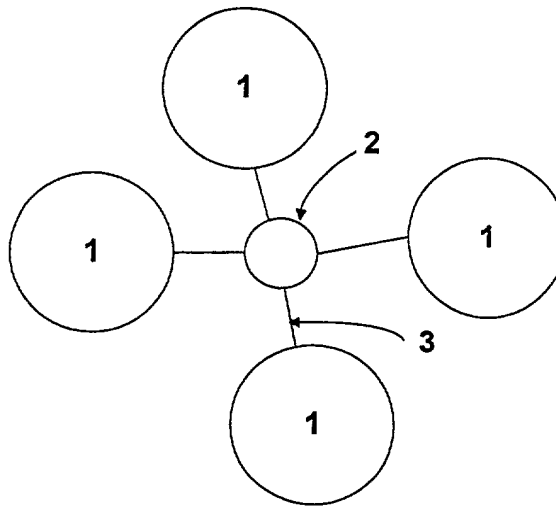


FIGURE 30B

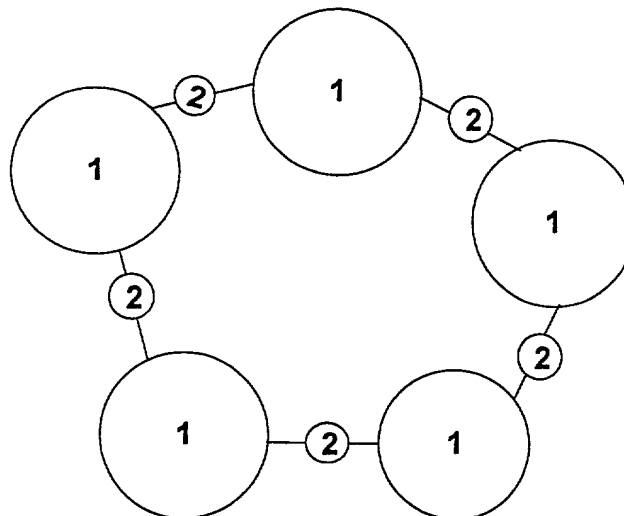


FIGURE 30C

28/30

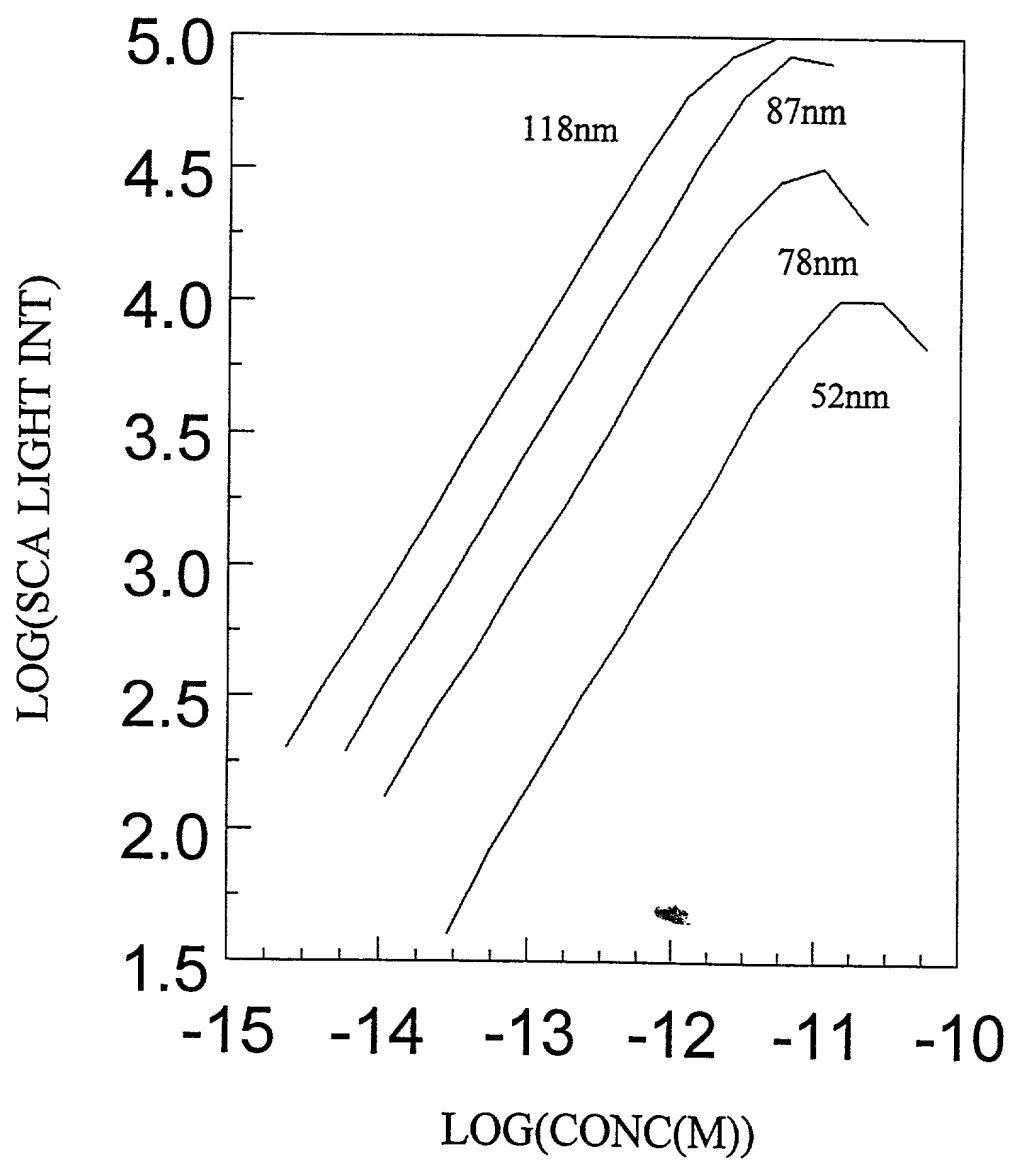


FIGURE 31

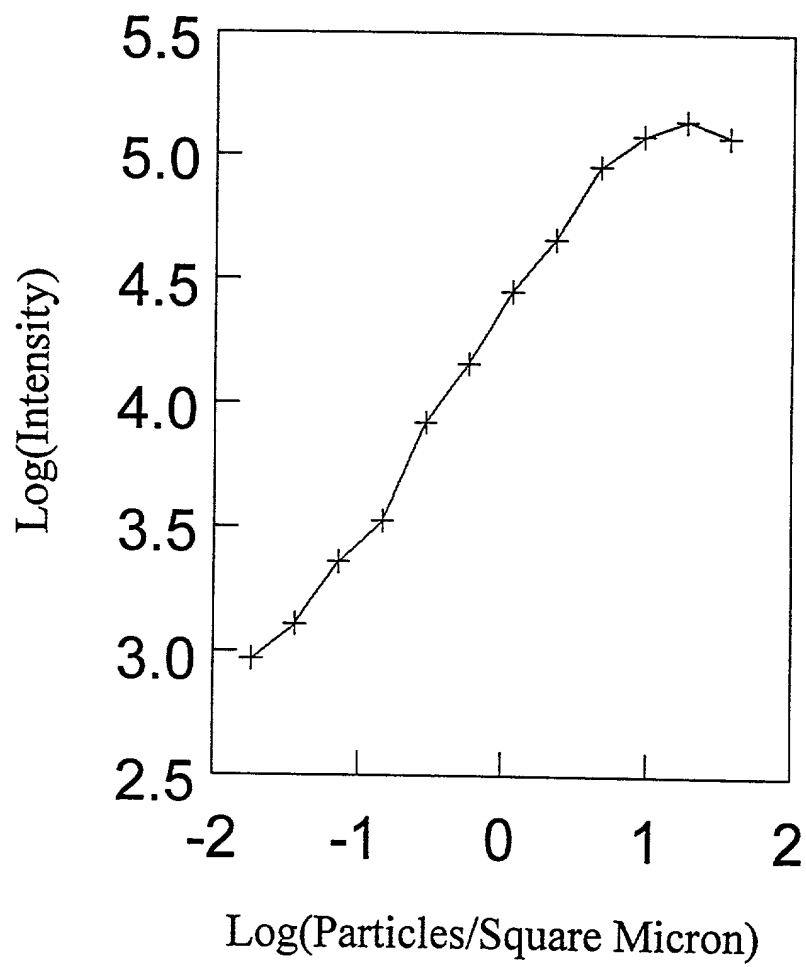


FIGURE 32

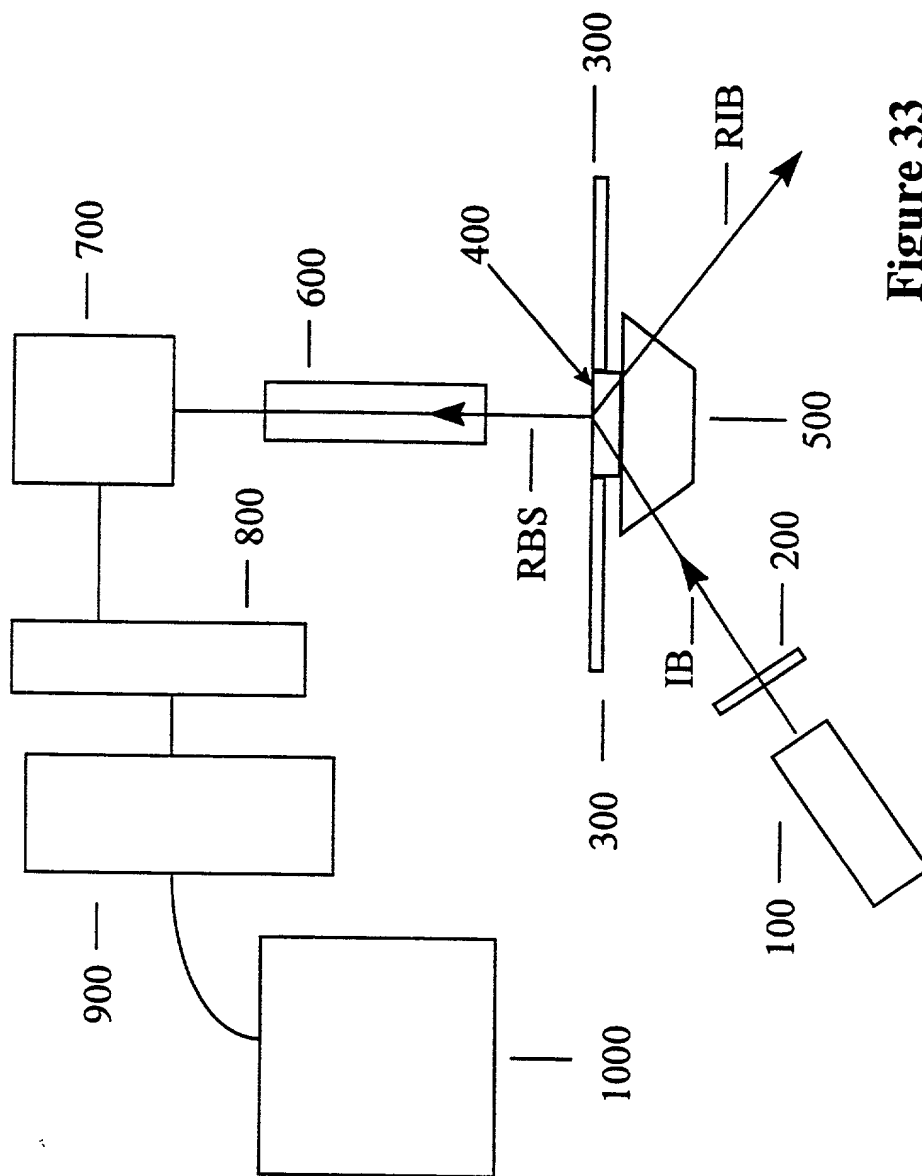


Figure 33